


300MHz DDS Signal Generator

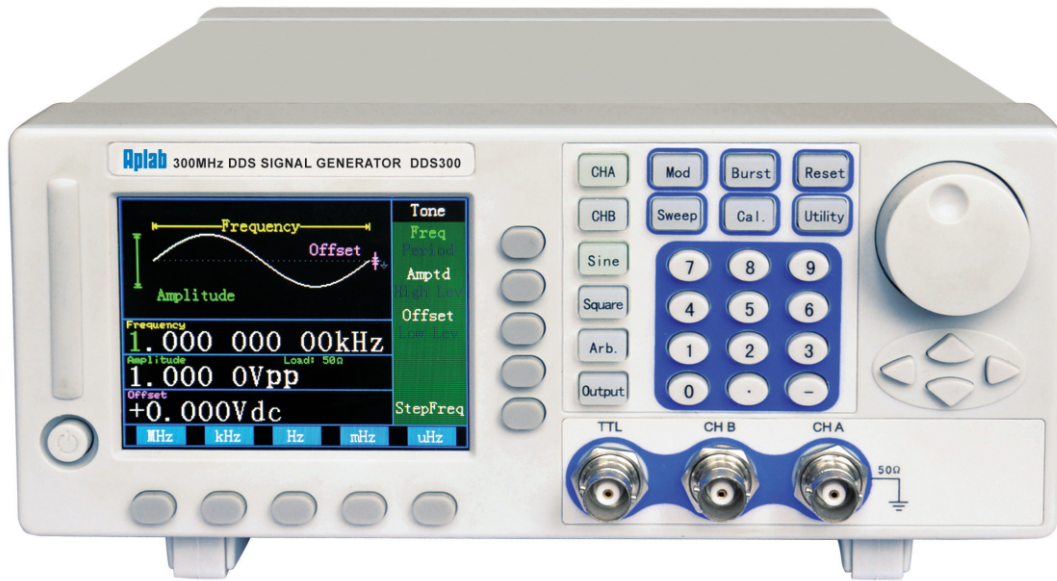

Features

- 300MHz Maximum Frequency
- 1 ppm High Accuracy, Less Distortion
- Double Independent Outputs
- AM, FM, FSK, PSK Modulation
- User can set accurate pulse width, burst signal as numbers
- USB Device, RS-232

Technical Specifications

CH A	
Frequency	
Range	Sine : 1 μ Hz ~ 300MHz Square : 1 μ Hz - 80MHz.
Resolution	1 μ Hz (Carrier Frequency \leq 80MHz) 1Hz (Carrier Frequency $>$ 80MHz).
Accuracy	\pm 1 ppm, Frequency $>$ 1.0 KHz. \pm 50 ppm, Frequency $<$ 1.0KHz.
Sine Output Level	
Range	-127dBm ~ +13dBm (-127dBm ~ -117dBm typical).
Resolution	0.1dB.
Accuracy	Setting \pm 1dBm (Output level \geq -105dBm). Setting \pm 2dBm (Output level \geq -117dBm).
Stationary Wave Ratio (SWR)	$<$ 1%.
Sine Spectrum Purity	
Harmonic	$<$ -30dBc.
Non-Harmonic	$<$ -40dBc.
Remain Modulating Frequency	$<$ 100Hz (BW : 0.3 ~ 3KHz, RMS $<$ 110MHz).
Square	
Rise / Fall Edge Time	\leq 15ns.
Overshoot	\leq 5%.

Modulation	
Type	AM, FM, FSK, PSK
External Modulation Input	Voltage Range : $\pm 2.5V$, Frequency : DC to 10KHz.
Frequency Sweep	
Sweep Rate	1 ms ~ 800s Linear (Carrier \leq 80MHz). 100ms ~ 800 s Logrithm (Carrier \leq 80MHz).
Sweep Range	100 μ Hz ~ 300MHz.
Step Time	10 ms ~ 800s (Carrier > 80MHz)
Burst	
Burst Count	1 ~ 10000 cycles
Internal	0.1ms ~ 800s.
CH B	
Frequency	
Range	1 μ Hz ~ 10MHz.
Resolution	1 μ Hz.
Accuracy	± 1 ppm, Frequency \geq 1.0KHz ± 50 ppm, Frequency < 1.0KHz.
Waveform	
Type	Sine, Square, Ramp, Pulse, Sinc, Exp, Noise, DC
Square	Edge Time : $\leq 50ns$. Duty Cycle : 0.01% ~ 99.99%
Pulse	Edge Time : $\leq 50ns$. Pulse Width : 200ns ~ 20s.
Ramp	Symmetry : 0.0% ~ 100.0%.
Output	
Amplitude	1mVpp to 10Vpp (50 ohms), 2mVpp to 20Vpp (High Z).
Offset	$\pm 5Vpk$ ac+dc (50 ohms), $\pm 10Vpk$ ac + dc (High Z).
General Characteristics	
Power	AC 220 (1 $\pm 10\%$)V, 50 (1 $\pm 10\%$)Hz, <40VA.
Dimension	254 x 103 x 374 mm.
Weight	3.8 Kg. approx.
Standard Accessories	
Power Cord	1 No.
BNC Testing Cable	1 No.
CD (Software + User's Guide)	1 No.
Optional Accessory	GPIB.

WE PURSUE A POLICY OF CONTINUOUS DEVELOPMENT AND PRODUCT IMPROVEMENT. THUS THE SPECIFICATIONS IN THIS DOCUMENT AND THE LOCATION OF CONTROLS ON THE FRONT PANEL MAY BE CHANGED WITHOUT NOTICE.

Aplab Test & Measurement Instruments Division

Aplab Limited, A-5, Wagle Estate, Thane 400 604. India. Tel. : 91-22-67395555, 25821861 Fax : 25823137 Email : tmsales@aplab.com

•AGRA •AHMEDABAD •BANGALORE •CHANDIGARH •CHENNAI •COIMBATORE •INDORE •JAIPUR •KOLKATA •LUCKNOW •MUMBAI •NEW DELHI •PUNE •SECUNDERABAD •THIRUVANANTHAPURAM